



Globe Pulsed Field System

Technological description

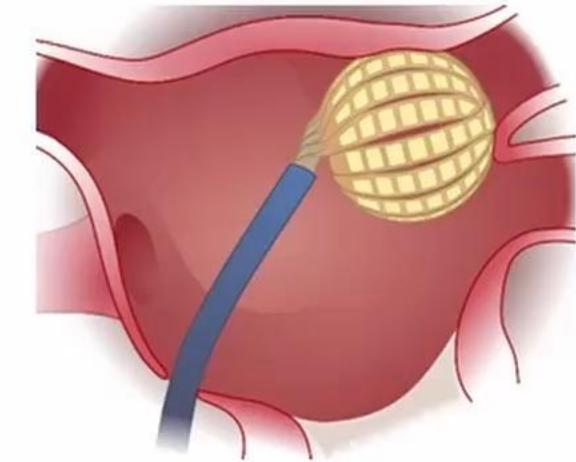

- 30 mm array
- 122 electrodes
- Mapping, ablation, pacing
- 3D mapping and navigation
- Contact mapping
- Voltage
- Activation
- Single-shot PVI
- Posterior Wall Isolation
- Mitral line
- Substrate ablation

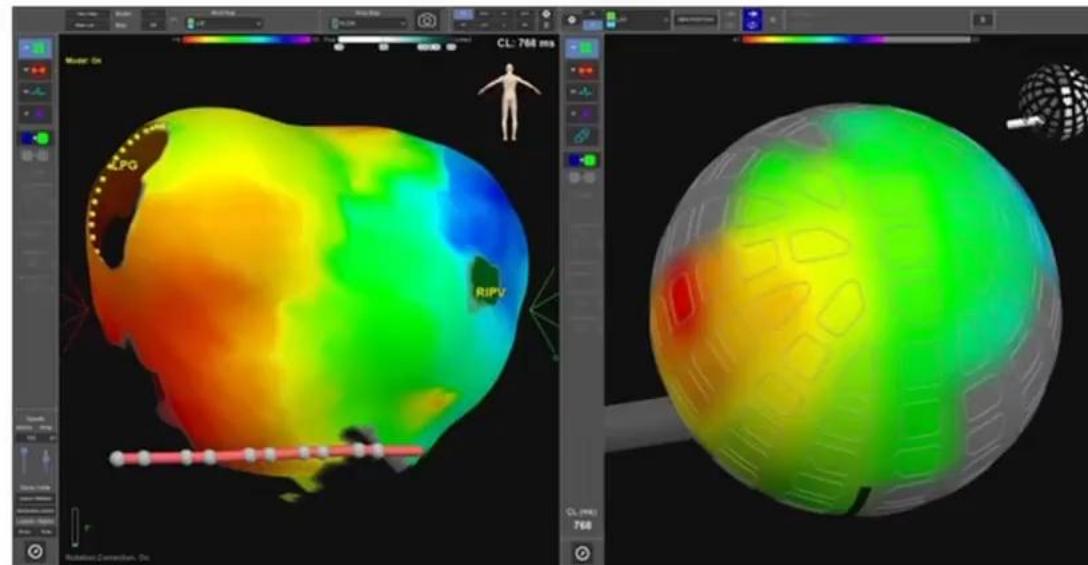

MOUNT SINAI
SCHOOL OF
MEDICINE



MOUNT SINAI
SCHOOL OF
MEDICINE